

WOCA A battery powered wound pump designed for use in low-resource settings

Nicolai, Noa; Diehl, J.C.; Raaijmakers, E.R.L.; Knulst, A.J.; Maharjan, Suraj

Publication date

2023

Document Version

Final published version

Citation (APA)

Nicolai, N., Diehl, J. C., Raaijmakers, E. R. L., Knulst, A. J., & Maharjan, S. (2023). *WOCA A battery powered wound pump designed for use in low-resource settings*. Poster session presented at Technical innovations in Medicine Congress 2023, Utrecht, Netherlands.

Important note

To cite this publication, please use the final published version (if applicable). Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy

Please contact us and provide details if you believe this document breaches copyrights. We will remove access to the work immediately and investigate your claim.

Green Open Access added to TU Delft Institutional Repository

'You share, we take care!' - Taverne project

<https://www.openaccess.nl/en/you-share-we-take-care>

Otherwise as indicated in the copyright section: the publisher is the copyright holder of this work and the author uses the Dutch legislation to make this work public.



WOCA

A battery powered wound pump designed for use in low-resource setting

Noa Nicolai, Eileen Raaijmakers, Arjan Knulst, Suraj Maharjan, Jenny Dankelman, Jan-Carel Diehl

SYNOPSIS

Vacuum-Assisted wound care (VAC) is effective for treating complex wounds, but is hardly available in low-resource settings. An affordable, portable and safe VAC device was developed to treat patients with chronic and complex wounds: the Wound Care (WOCA) Pump. The WOCA safely controls the pressure accurately (+/- 10%) between -70 and -125 mmHg for a total component cost of USD 150. In this research important steps were taken to make VAC therapy more accessible, affordable and safe for marginalised patients in low-resource settings. Next research will aim to assess its safe clinical use.

INTRODUCTION

In Low-Middle Income Countries (LMICs) the prevalence of complex wounds is alarmingly high. Complex wounds have a significant impact on the health and quality of life of the patient and their families. Vacuum-assisted wound closure (VAC) is a widely used treatment in the developed world to treat chronic and complex wounds. However, due to the high costs and low availability of the commercially available devices, VAC therapy is not a treatment option for many patients in LMICs.

AIM

The aim of this study is to develop a low-cost, portable VAC device to make the treatment more accessible for LMICs.



Figure 3: Current situation in the design context, using the AquaVAC.

METHOD

First, extensive context analysis, literature and expert review was done to compile a set of requirements and design guidance for the VAC device. Secondly, a conceptual design for a low-cost device was made, which meets all the requirements. Next, the conceptual design was transformed into a functional prototype in the Green Pastures Hospital (GPH) in Nepal. Finally, requirement validation was performed and a demonstration was given to the medical staff to evaluate additional wishes of the end-users.

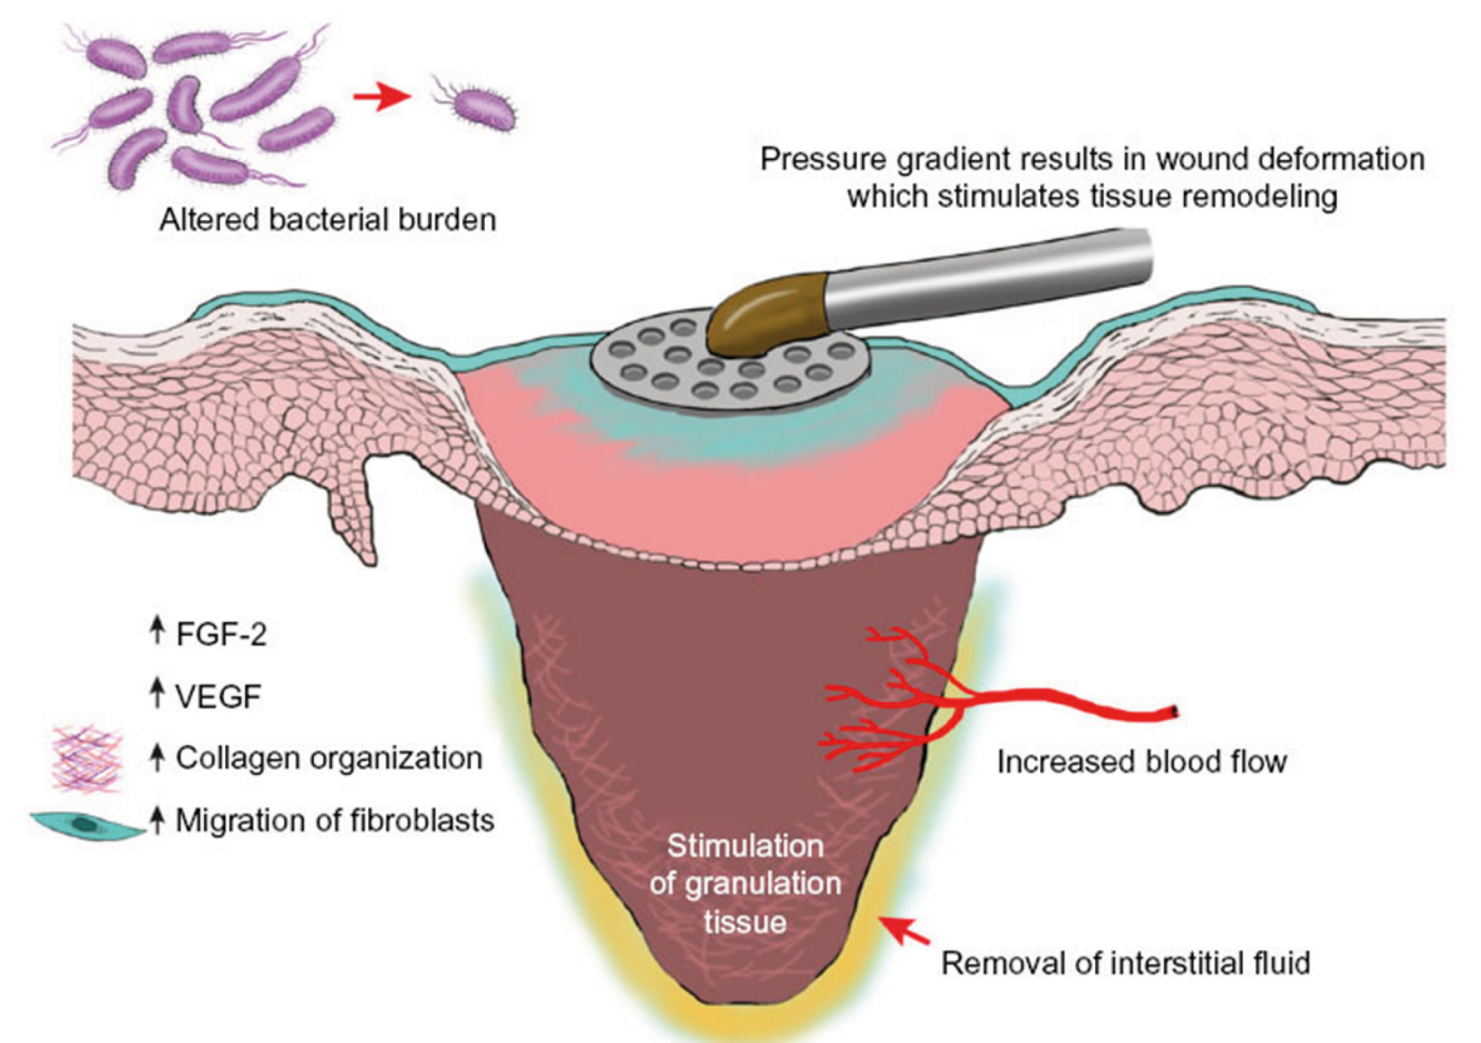


Figure 2: Negative Pressure Wound Therapy (NPWT) beneficial effects.



Figure 1: Design context. International Nepal Fellowship (INF), Green Pastures Hospital (GPH), Pokhara, Nepal

RESULTS

Analysis of the market:

Unnecessarily costly
Low-cost solutions lack reliability, safety and ease of use.

Wound Care (WOCA) Pump

Conceptual design

- Includes **automatic** pressure control
- Compatible** with self-made dressings and standard canisters
- Portable** design, battery last for 15 hours
- Simple** interface, enables smooth operation & monitoring
- Easy** to repair, consists of widely available, replaceable components

The conceptual design was transformed to a functional design and developed in the GPH. Features like automatic pressure control and safety alarms were added using Arduino Program-ming.

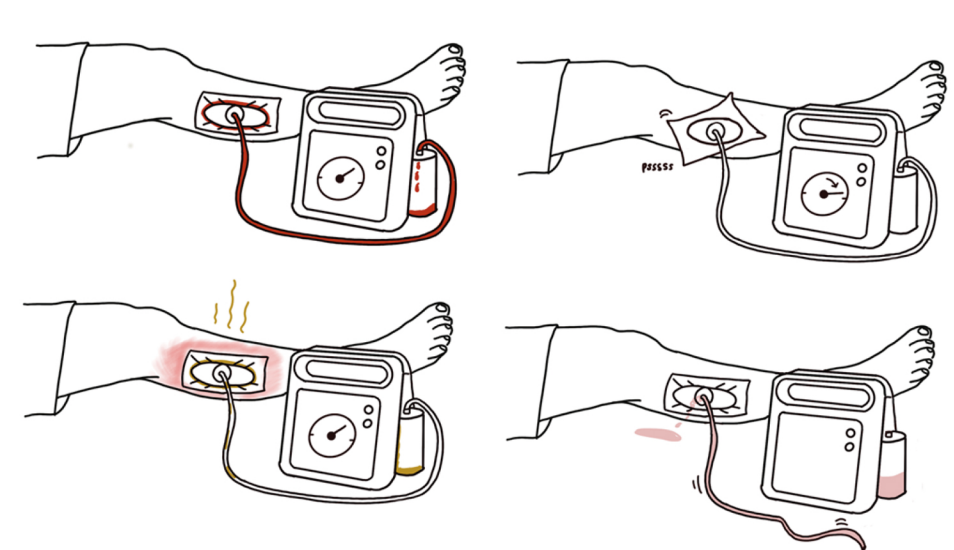


Figure 5: Safety concerns: 1. Pressure lost; 2. Bleeding; 3. Infection; 4. Tube blockage/tube disconnection.

Production costs: < 150 US Dollars

Compatible with inhouse made dressings of less than 1 USD. The pressure can be set in a range between -70 and -125 mmHg and is regulated within the allowable margin of 10% of the set pressure. The pump was able to overcome an air leak ratio of more than 1200 mL/min. The device includes a rechargeable battery that lasts for at least one therapy cycle (3-5 days). The components are available from local stores or can be delivered to the hospital from (local) online platforms. Furthermore, the housing can be printed with the 3D printer located in the GPH.

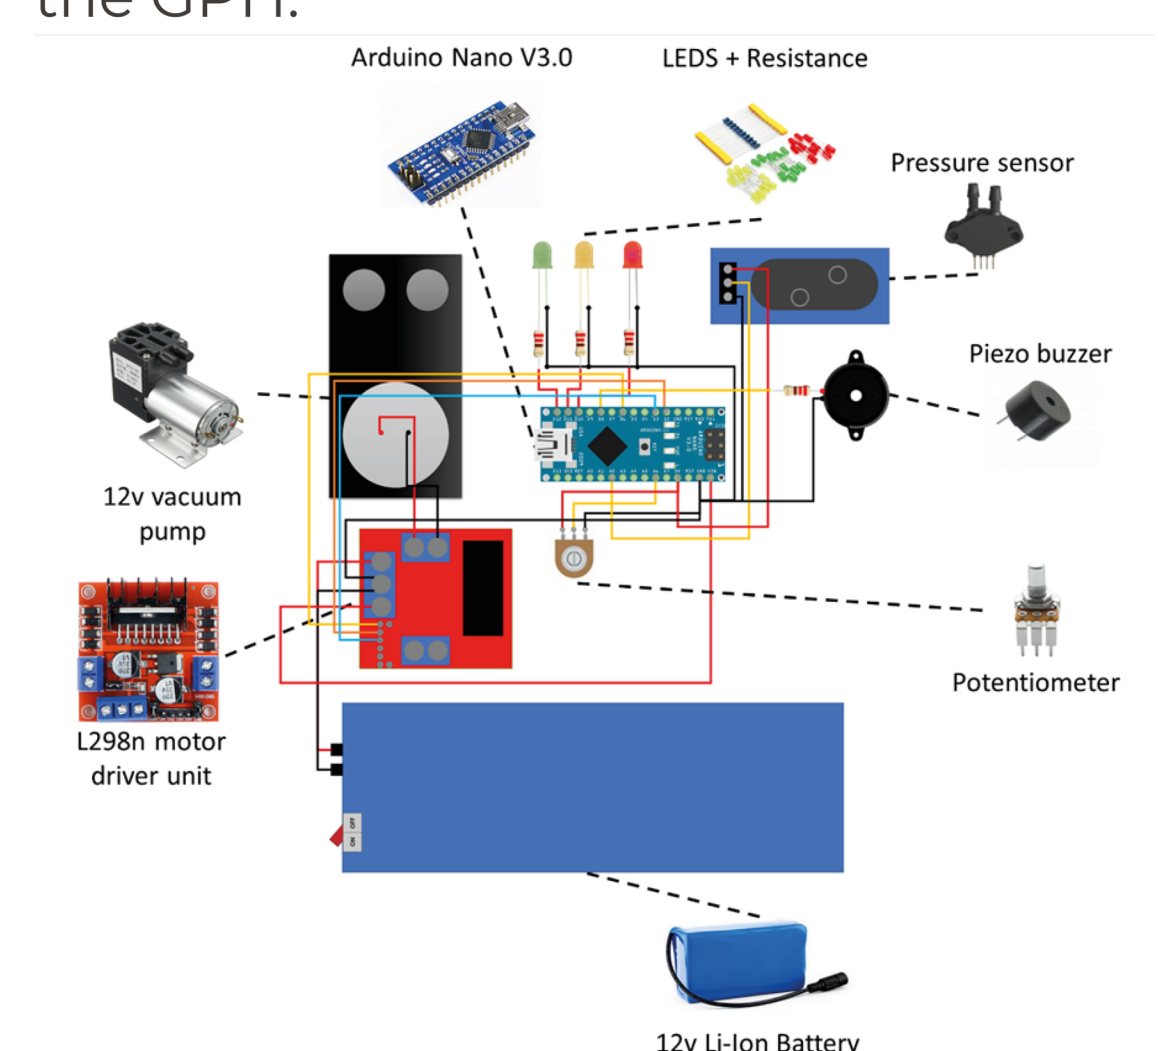


Figure 6: Electrical circuit design to power the vacuum device.

CONCLUSION

A functional, portable, simple and easy to repair VAC device has been developed. The WOCA Pump is made from widely available components, is compatible with self-made dressings, and can be developed for less than 150 USD. A clinical trial is being prepared to validate the safety and functionality of the next iteration of the device in the clinic. The development of the WOCA will provide a sustainable solution to make wound care more affordable and accessible in LMICs.

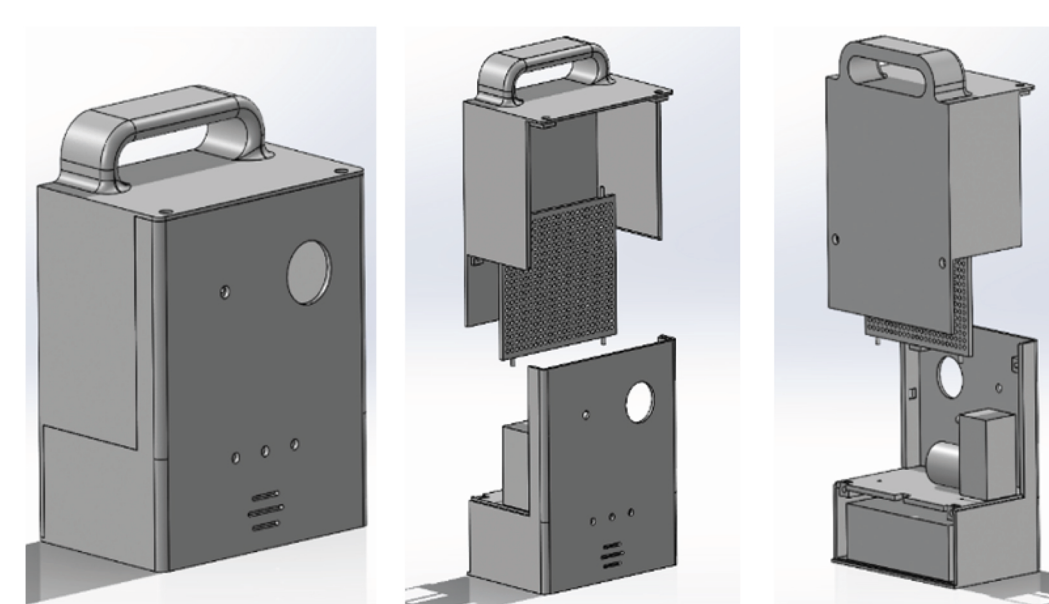


Figure 7: Functional design housing.

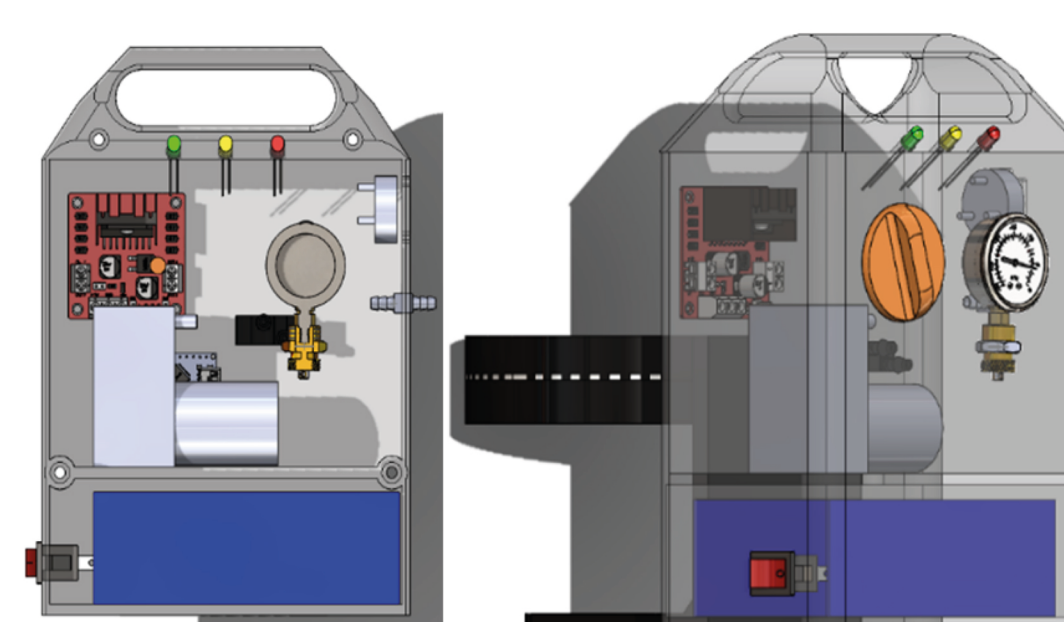


Figure 8: Arrangement of the components inside the housing.

FUTURE STEPS

- Design iteration
- Overflow protection system
- Safety optimisation
- Durability testing
- ISO norm validation
- Clinical testing
 - WOCA vs AquaVAC
 - WOCA vs devices available from the market
- World wide local production

REFERENCES

- [1] K. Järbrink et al., "Prevalence and incidence of chronic wounds and related complications: A protocol for a systematic review," *Syst Rev*, vol. 5, no. 1, pp. 1-6, Sep. 2016, doi: 10.1186/s13643-016-0329-Y/TABLES/1.
- [2] A. J. Knulst et al., "Directions for surgical capacity developments in Nepal: a population-based assessment," *Trop Med Int Health*, vol. 24, no. 9, pp. 1128-1137, Sep. 2019, doi: 10.1111/TMI.13292.
- [3] E. Raaijmakers, "Design of a low-cost device for Negative Pressure Wound Therapy in low and middle-income countries." 2022. Accessed: Feb. 08, 2023. [Online]. Available: <https://repository.tudelft.nl/islandora/object/uuid%3A35d644fe-900d-4c52-80eb-6b1398250035>
- [4] D. Parida, "AC Fan Speed Control using Arduino and TRIAC," Feb. 05, 2020. <https://circuitdigest.com/microcontroller-projects/ac-fan-speed-control-using-arduino-and-triac> (accessed Feb. 09, 2023).
- [5] M. M.J, A. L.C, S.-B. El, and M. W., "Vacuum-assisted closure: a new method for wound control and treatment: animal studies and basic foundation," *Ann Plast Surg*, vol. 38, no. 6, pp. 837-840+877, Dec. 1997, doi: 10.1097/0000637-199706000-00001.
- [6] L. C. Argenta and M. J. Morykwas, "Vacuum-assisted closure: a new method for wound control and treatment: clinical experience," *Ann Plast Surg*, vol. 38, no. 6, pp. 563-76; discussion 577, Jun. 1997, doi: 10.1097/0000637-199706000-00002.
- [7] K. N. Lee, M. Ben-Nakhi, E. J. Park, and J. P. Hong, "Cyclic negative pressure wound therapy: an alternative mode to intermittent system," *Int Wound J*, vol. 12, no. 6, p. 686, Dec. 2015, doi: 10.1111/IWJ.12201.
- [8] A. Sogorski et al., "Superior Enhancement of Cutaneous Microcirculation Due to 'Cyclic' Application of a Negative Pressure Wound Therapy Device in Humans - Local and Remote Effects," *Front Surg*, vol. 9, Mar. 2022, doi: 10.3389/FSURG.2022.822122.